



Prior to use, carefully read the instructions for use.

EN

**GC Fuji ORTHO™ BAND LC PASTE PAK
(Automix Compatible)**

DUAL CURED REINFORCED GLASS INOMER ORTHODONTIC BAND CEMENT

For use only by a dental professional in the recommended indications.

RECOMMENDED INDICATIONS

- Cementation of orthodontic bands
- Orthodontic bands retained with stainless steel crowns (e.g. Herbst or expansion appliances)

CONTRAINDICATIONS

Avoid use of this product in patients with known allergies to glass ionomer cement, methacrylate monomer or methacrylate polymer.

IDENTIFICATION OF PARTS (Fig. 1)

- Cover 2. Inner plunger 3. Cartridge tip 4. Lever 5. Adjusting guide 6. Lever 7. Sliding block 8. Piston release 9. Grip For LC (Available separately) 10. Release tab 11. Guide Pin

PASTE PAK CARRYING LOAD

Make sure that the piston is completely retracted into the dispenser (Fig. 2).

NOTE:

When carrying the piston, push the piston release and at the same time pull the sliding block (on the underside of the dispenser) with fingers.

2. Load the cartridge into the Paste Pak Dispenser (Fig. 3). Ensure the **m** mark on the cartridge lines up with the **M** mark on the Paste Pak Dispenser (Fig. 4). Then turn the cartridge fully to the right position.

3. After cartridge loading, push the piston release forward until it stops.

NOTE:

To remove the piston, return the piston fully and turn the cartridge back to the parked position.

DIRECTIONS FOR USE**1. TOOTH PREPARATION**

Always ensure the tooth to be cemented is cleaned with pumice and water, then rinsed with water. Remove excess moisture by blotting with a cotton pellet or gently blowing with an air-free air.

DENTOCERATE® Prepare the tooth surface to be cemented should appear smooth (NOTE).

The surface to be bonded contains porcelain, zirconium ceramic or metal, porcelain should be sandblasted and pre-treated with silane, any other metal should be sandblasted. Refer to manufacturer's instructions.

2. PREPARATION OF THE CARTRIDGE

Make sure that the band is prepared and handled according to the manufacturer's instructions.

3. LOAD THE CARTRIDGE

a) Remove the cartridge cover.

b) Depress the lever to dispense the required amounts of paste.

NOTE:

After dispensing the first time from a new cartridge or after a long interval in storage, bleed the pastes from the piston.

2. The adjusting guide is moved forwards or backwards to change the quantity of material to be dispensed (Fig. 5).

3. Depress the lever while holding the cartridge and dispenser (Fig. 6). After dispensing the lever (Fig. 7), level 1, level 2, level 3, etc., are dispensed sequentially.

4. After dispensing, spread the two pastes thinly on the mixing tip (Fig. 8) and replace the cartridge cover.

5. After dispensing, spread the two pastes thoroughly, with light strokes, 3-4 seconds.

NOTE:

To mix the two pastes, repeat the dispensing until the cartridge is full.

6. Do not mix GC Fuji ORTHO BAND LC PASTE PAK with any other adhesive.

7. 3-DISPENSING AND AUTOMIXING WITH GC MIXING TIP For LC

Make sure that the band is prepared and handled according to the manufacturer's instructions.

8. REMOVING THE CARTRIDGE

After dispensing the first time from a new cartridge or after a long interval in storage, bleed the pastes from the piston.

2. The adjusting guide is moved forwards or backwards to change the quantity of material to be dispensed.

3. Depress the lever while holding the cartridge and dispenser (Fig. 6). After dispensing the lever (Fig. 7), level 1, level 2, level 3, etc., are dispensed sequentially.

4. After dispensing, spread the two pastes thinly on the mixing tip (Fig. 8) and replace the cartridge cover.

5. After dispensing, spread the two pastes thoroughly, with light strokes, 3-4 seconds.

NOTE:

To mix the two pastes, repeat the dispensing until the cartridge is full.

6. Do not mix GC Fuji ORTHO BAND LC PASTE PAK with any other adhesive.

7. CLEANING / STERILIZATION OF PASTE PAK DISPENSER

For cleaning and sterilization of PASTE PAK DISPENSER, refer to the respective instructions for use.

SHADE

Blue

STORAGE

Recommended for optimal performance, store in a cool and dark place (4-25°C) (39-77°F).

If stored for a prolonged period of time, store in refrigerator.

PACKAGE

1) GC Fuji ORTHO BAND LC PASTE PAK (Automix Compatible)

Refill Package Paste Pack Cartridge (12.9g / 7.2ml) (2).

2) Paste Pak Dispenser (1).

3) GC MIXING TIP For LC (20)

CAUTION

1. In case of contact with oral tissue or skin, remove immediately with a sponge or cotton soaked in alcohol. Flush with water. To avoid to contact with oral tissue or skin, do not use the product if it has been used to contact with eyes, flush immediately with water and seek medical advice.

3. In rare cases metal may cause sensitivity to some people. If any reaction occurs, discontinue the use of the product. If any such reactions are experienced, discontinue the use of the product. Please refer to the product information leaflet (PPE) such as gloves, face mask and safety shower gels always be worn.

Some products referred in the present IFU may be classified as hazard class IIb according to GHS. Always familiarize yourself with the safety data sheets available at <http://www.gecure.com>.

This product is supplied by your supplier.

CLEANING AND DISINFECTION

MULTI-USE DELIVERY SYSTEMS: To avoid cross-contamination between patients this device requires mid-level disinfection. Immediately after use, clean and sterilize the device. Discard if damaged.

DO NOT REUSE. Thoroughly clean device to prevent drying and accumulation of contaminants. Disinfect with a mid-level registered healthcare infection control product according to regional/national guidelines.

Use caution - Reporting:

If you become aware of any kind of undesired effect, reaction or similar events experienced by use of the product, including those not listed in this document, please report them to the relevant national vigilance system, selecting the proper authority of your country accessible via https://ec.europa.eu/euroveil/sectors/medical-devices/contactas_en. In this way will contribute to improve the safety of this product.

Last revised: 06/2019



Prior to use, carefully read the instructions for use.

EN

Prior to use, carefully read the instructions for use.

BG

**GC Fuji ORTHO™ BAND LC PASTE PAK
(Automix Compatible)**

DUAL CURED REINFORCED GLASS INOMER ORTHODONTIC BAND CEMENT

For use only by a dental professional in the recommended indications.

RECOMMENDED INDICATIONS

- Cementation of orthodontic bands
- Orthodontic bands retained with stainless steel crowns (e.g. Herbst or expansion appliances)

CONTRAINDICATIONS

Avoid use of this product in patients with known allergies to glass ionomer cement, methacrylate monomer or methacrylate polymer.

IDENTIFICATION OF PARTS (Fig. 1)

- Cover 2. Inner plunger 3. Cartridge tip 4. Lever 5. Adjusting guide 6. Lever 7. Sliding block 8. Piston release 9. Grip For LC (Available separately) 10. Release tab 11. Guide Pin

PASTE PAK CARRYING LOAD

Make sure that the piston is completely retracted into the dispenser (Fig. 2).

NOTE:

When carrying the piston, push the piston release and at the same time pull the sliding block (on the underside of the dispenser) with fingers.

2. Load the cartridge into the Paste Pak Dispenser (Fig. 3). Ensure the **m** mark on the cartridge lines up with the **M** mark on the Paste Pak Dispenser (Fig. 4).

3. After cartridge loading, turn the cartridge fully to the right position.

4. After cartridge loading, push the piston release forward until it stops.

NOTE:

To remove the piston, return the piston fully and turn the cartridge back to the parked position.

DIRECTIONS FOR USE**1. TOOTH PREPARATION**

Always ensure the tooth to be cemented is cleaned with pumice and water, then rinsed with water. Remove excess moisture by blotting with a cotton pellet or gently blowing with an air-free air.

DENTOCERATE® Prepare the tooth surface to be cemented should appear smooth (NOTE).

The surface to be bonded contains porcelain, zirconium ceramic or metal, porcelain should be sandblasted and pre-treated with silane, any other metal should be sandblasted. Refer to manufacturer's instructions.

2. PREPARATION OF THE CARTRIDGE

Make sure that the band is prepared and handled according to the manufacturer's instructions.

3. LOAD THE CARTRIDGE

a) Remove the cartridge cover.

b) Depress the lever to dispense the required amounts of paste.

NOTE:

After dispensing the first time from a new cartridge or after a long interval in storage, bleed the pastes from the piston.

2. The adjusting guide is moved forwards or backwards to change the quantity of material to be dispensed (Fig. 5).

3. Depress the lever while holding the cartridge and dispenser (Fig. 6). After dispensing the lever (Fig. 7), level 1, level 2, level 3, etc., are dispensed sequentially.

4. After dispensing, spread the two pastes thinly on the mixing tip (Fig. 8) and replace the cartridge cover.

5. After dispensing, spread the two pastes thoroughly, with light strokes, 3-4 seconds.

NOTE:

To mix the two pastes, repeat the dispensing until the cartridge is full.

6. Do not mix GC Fuji ORTHO BAND LC PASTE PAK with any other adhesive.

7. CLEANING / STERILIZATION OF PASTE PAK DISPENSER

For cleaning and sterilization of PASTE PAK DISPENSER, refer to the respective instructions for use.

SHADE

Blue

STORAGE

Recommended for optimal performance, store in a cool and dark place (4-25°C) (39-77°F).

If stored for a prolonged period of time, store in refrigerator.

PACKAGE

1) GC Fuji ORTHO BAND LC PASTE PAK (Automix Compatible)

Refill Package Paste Pack Cartridge (12.9g / 7.2ml) (2).

2) Paste Pak Dispenser (1).

3) GC MIXING TIP For LC (20)

CAUTION

1. In case of contact with oral tissue or skin, remove immediately with a sponge or cotton soaked in alcohol. Flush with water. To avoid to contact with oral tissue or skin, do not use the product if it has been used to contact with eyes, flush immediately with water and seek medical advice.

3. In rare cases metal may cause sensitivity to some people. If any reaction occurs, discontinue the use of the product. If any such reactions are experienced, discontinue the use of the product. Please refer to the product information leaflet (PPE) such as gloves, face mask and safety shower gels always be worn.

Some products referred in the present IFU may be classified as hazard class IIb according to GHS. Always familiarize yourself with the safety data sheets available at <http://www.gecure.com>.

This product is supplied by your supplier.

CLEANING AND DISINFECTION


MULTI-USE DELIVERY SYSTEMS: To avoid cross-contamination between patients this device requires mid-level disinfection. Immediately after use, clean and sterilize the device. Discard if damaged.

DO NOT REUSE. Thoroughly clean device to prevent drying and accumulation of contaminants. Disinfect with a mid-level registered healthcare infection control product according to regional/national guidelines.

Use caution - Reporting:

If you become aware of any kind of undesired effect, reaction or similar events experienced by use of the product, including those not listed in this document, please report them to the relevant national vigilance system, selecting the proper authority of your country accessible via https://ec.europa.eu/euroveil/sectors/medical-devices/contactas_en. In this way will contribute to improve the safety of this product.

Last revised: 06/2019

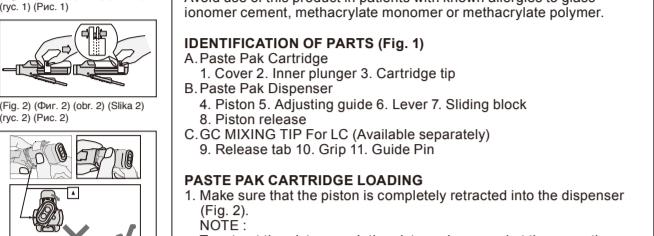

Prior to use, carefully read the instructions for use.

EN

**GC Fuji ORTHO™ BAND LC PASTE PAK
(Automix Compatible)**

DUAL CURED REINFORCED GLASS INOMER ORTHODONTIC BAND CEMENT K FIXACI ORTOPEDICKÝM KROZU

Cementaci na stálej krovce s využitím skloinomeru

VYKONÁVANÍ

Určeno využívať k použitiu na stomatologickej praxi v doporučených indikáciach.

PRERUČENÉ INDIKÁCIE

- Cementacia na ortodontické bandy
- Cementacia na ortodontické bandy s upevnením pomocou kovových kružníkov

KONTRAINDIKÁCIE

Neplatí sa na dospelých pacientov s alergiami na cement, metakrilátne monomer alebo metakrilátový polymer.

OPAKOVANÉ INDIKÁCIE

1. Využívanie na výrobu a upevnenie ortodontických bandových kru

